

The image contains three separate diagrams of a water purifier, each with a label pointing to a specific part:

- Diagram 1 (Top):** Shows the top of the purifier with the lid open. Label **A** points to the outer housing. Label **B** points to the inner lid. Label **C** points to the side outlet pipe.
- Diagram 2 (Middle):** Shows the side of the purifier with a control panel. Label **D** points to the control panel.
- Diagram 3 (Bottom):** Shows the front of the purifier with a water tap. Label **E** points to the front panel.

A Coperchio
B Sistema di dosaggio del farmaco
C Corpo del nebulizzatore
D Boccaglio
E Unità di base

A diagram of a power tool, likely a drill, with labels a-f pointing to various components. Label 'a' points to the trigger switch. Label 'b' points to the battery pack. Label 'c' points to the battery pack. Label 'd' points to the battery pack. Label 'e' points to the battery pack. Label 'f' points to the drill bit.

- a** Pulsante di accensione/spegnimento
- b** LED per connessione wireless
- c** Pulsante di reset
- d** LED per auto-test
- e** LED di alimentazione
- f** LED del bocchaglio



Vectura Group Ltd
One Prospect West, Chippenham, Wiltshire, SN14 6FH,
Regno Unito
www.veectura.com
Vectura Ireland Limited
Block 2, Newtown Business and Enterprise Centre
Newtownmountkennedy
Co. Wicklow, A63 XV26
Ireland



CE 0123



08CN0215
020522

1

2

3

The diagram consists of three numbered steps illustrating the charging process:

- Step 1:** A black arrow points to the USB port on the side of the device, indicating where to plug the cable. A red battery icon is shown to the right.
- Step 2:** The USB cable is plugged into the device. A green battery icon with the text "4 h" next to it is shown to the right, indicating the charging time.
- Step 3:** The USB cable is plugged into the device. A fully charged green battery icon is shown to the right, indicating the device is ready for use.

[illegible]



Sistema di inalazione

Scheda di riferimento rapido






Il presente documento è una Scheda di riferimento rapido. Per una descrizione dettagliata, leggere le istruzioni per l'uso.




Riempimento del nebulizzatore

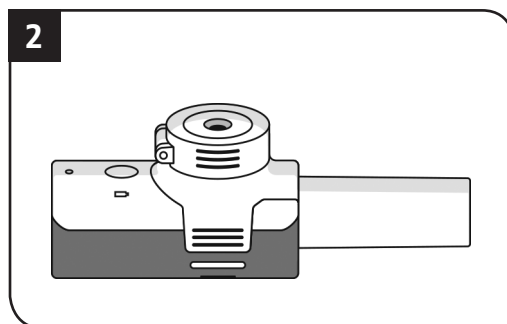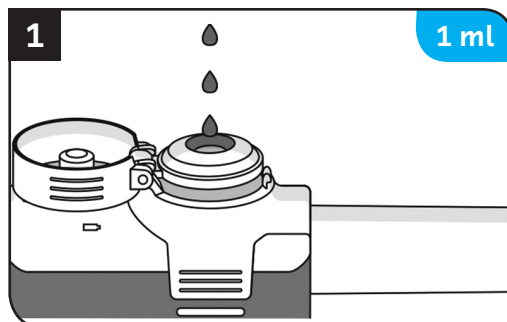




Inalazione

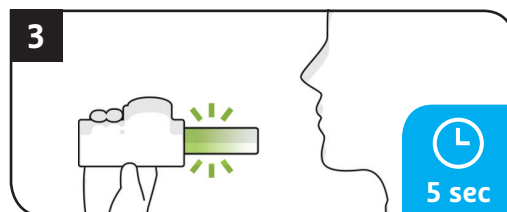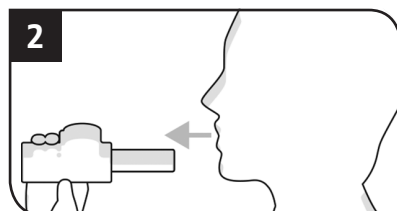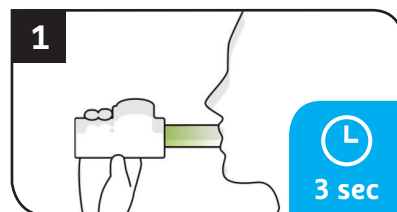



Risciacquo immediato

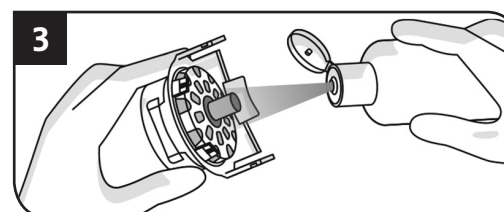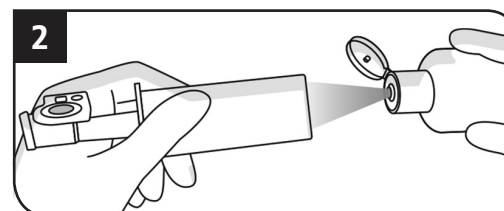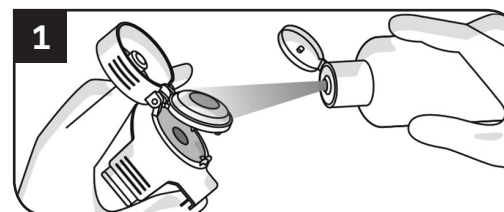





Pulizia settimanale

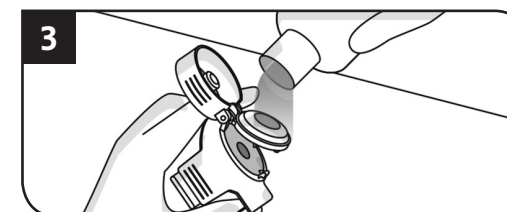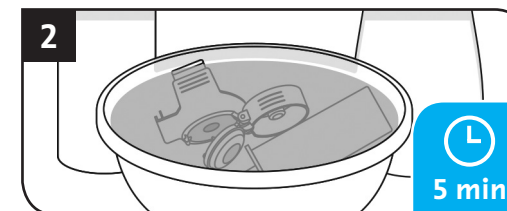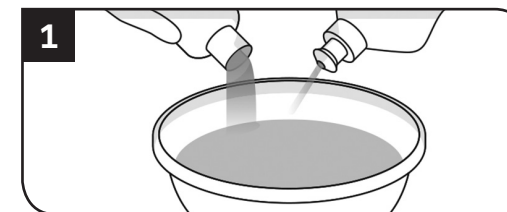

Disinfezione settimanale

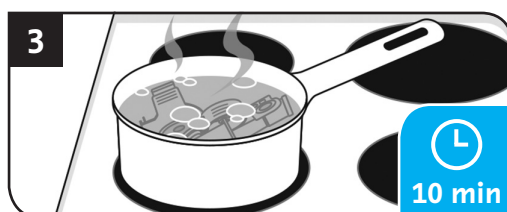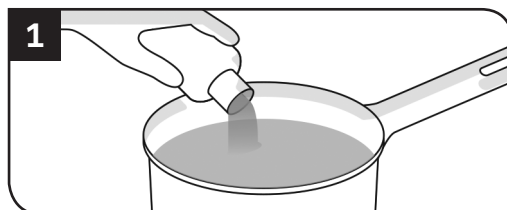

Asciugatura

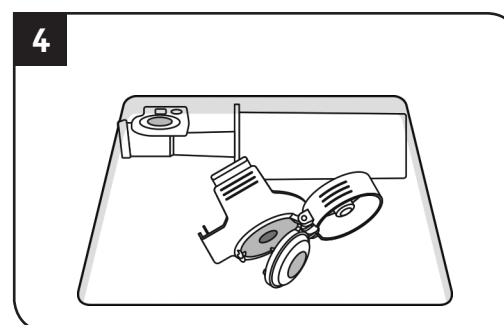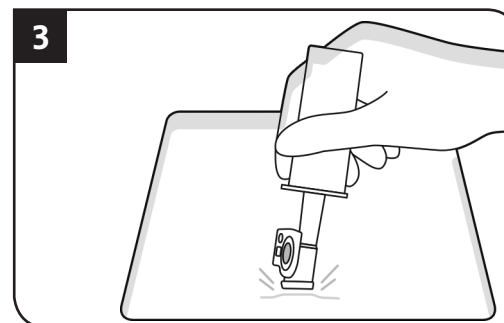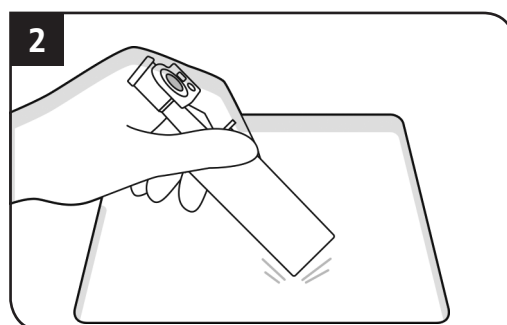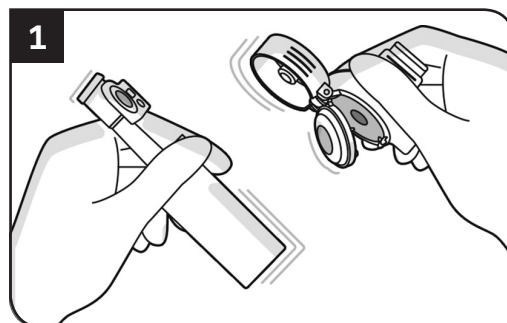

Note

[illegible]

Bayer
88870638